
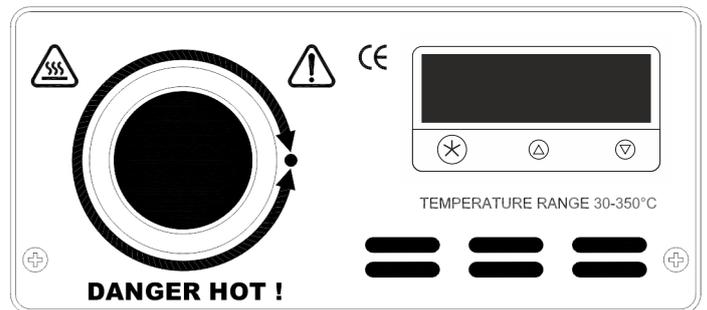


Quick-CAL Range

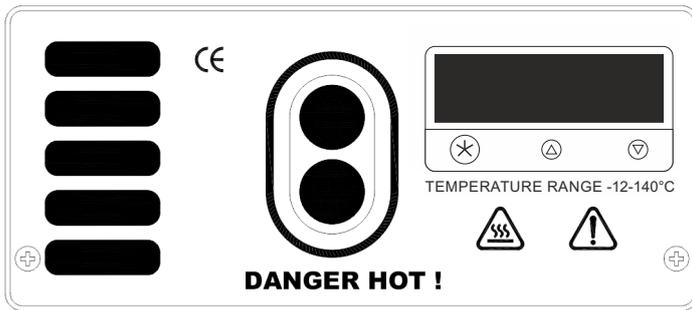

The Quick-Cal range are designed to be fast, simple to use and above all truly portable. Ideal for the simple testing of temperature sensors.

OPERATION

Altering the Block Temperature, (Setpoint)

1. Switch the unit on. The power switch is located on the rear panel.
2. The controller will briefly show its software version before displaying an indication of the block temperature.



A. Heating beacon B. STAR button
C. Down button D. Up button E. Cooling beacon

3. Press the STAR button to display the current setpoint.
4. Holding down the STAR button, press either the up or down button to adjust to the desired setpoint.
5. Release the buttons and the display will revert to the current block temperature and store the new setpoint.

Altering the Ramp Rate

The ramp rate or set point rate limit provides a means of limiting the rate at which the temperature of the heat source will increase or decrease.

Normally it is desirable to allow the unit to heat and cool at the maximum rate possible, which is achieved by setting the ramp rate to OFF.

This is the Factory set default value. For some applications, e.g. testing temperature cut out switches it can be useful to be able to program the temperature ramp rate.

To alter the ramp rate:

Press both the up and down buttons at the same time for 3 seconds until **tunE** is displayed. Press the up button until **SPrr** is displayed. Now press the STAR button to display **OFF** while holding down the STAR button, press the UP button to display the desired setpoint ramp value.


The default ramp units are in °C/minute.



The other controller functions are hidden from the operator. The values are pre-set and should not be changed.

Getting Better Accuracy

For accurate calibration of sensors it is good practice to include a calibrated reference probe in the block, then the units under test are compared to this reference probe.

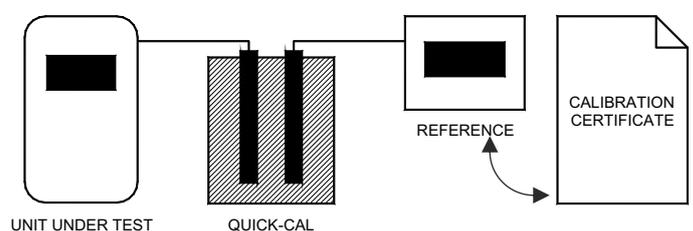



Safe Use

- Do not use in wet or damp environments.
- Care should be taken to avoid handling the calibration area when hot - Risk of Burns - Keep flammable items away.
- Cool before placing in carry case.
- No liquids should be used.
- Read this instruction leaflet before use.
- No user Serviceable parts, do not dismantle.
- Not for use in Hazardous Areas.
- Disconnecting device: The Quick-Cal can be isolated by removing the power cable.



Cautionary Note

Failure to follow these instructions could result in fatal injury or cause damage to the product.

Isotech products are intended for use by technically trained and competent personnel familiar with good measurement practices.

It is expected that personnel using this equipment will be competent with the management of apparatus which may be powered or under extremes of temperature, and are able to appreciate the hazards which may be associated with, and the precautions to be taken with, such equipment.

Unpacking and Initial Inspection

Our packing department uses custom designed packaging to send out your unit, after unpacking the unit, to inspect it for any sign of shipping damage, and confirm that your delivery is in accordance with the packing note. If you find any damage or that part of the delivery is missing please notify us or our agent, and the carrier immediately. If the unit is damaged you should keep the packaging for possible insurance assessment.

Electrical Supply

Before connecting to the electricity supply please familiarize yourself with the parts of this instruction sheet relevant to your model.

Your unit's supply voltage requirement is specified on a plate on the instrument along with the serial number. All instruments will work on an electricity supply frequency of 50Hz or 60Hz.

The Quick-Cal low is powered from a 15V D.C. Switch Mode power supply, or a 12V, 7Ah Battery.

Read ALL Handbooks supplied with Electrical Accessories before use.

Trouble Shooting

- Quick-Cal Low will not reach -12°C . . .
 - Check ambient temperature - Quick-Cal Low is rated for -12°C in an ambient of 20°C.
- Quick-Cal High will not control at 30°C . . .
 - Check ambient temperature - Quick-Cal High is rated for use at 30°C in an ambient of 20°C.
- Quick-Cal does not power up . . .
 - Check the switch position
 - Check the power supply
 - Check the connecting lead
 - Check fuse - the Quick-Cal high has a fuse in each supply line. Fuses are accessed by removing the front cover of the power entry module and locate in the removable red draw.

The temperature controller includes diagnostic alarms that warn if an internal error occurs in the controller.

Alarm	What It Means	What to Do
inPt: FAiL	Sensor Fail.	Return for Repair
dAtA: FAiL	Non-Volatile memory failure.	Return for Repair
hAnd: FAiL	Manual power failure.	Return for Repair
tunE: FAiL	Immediate fail on Autotune start. Fail later during cycle.	Power cycle and repeat process. If second attempt fails then return for repair.

Quick-CAL Blackbody

The Quick-CAL Blackbody is ideal for the rapid and portable testing of infra red thermometers. The cavity has dimensions of 25 x 115mm with an end cone. The emissivity is >0.99. The surface coating has an emissivity of 0.98 and the cavity geometry gives an overall emissivity > 0.99. No insert is used with this model - the cavity is used as the target for the infra red thermometer.



Quick Cal Low Temperature
-12°C to +140°C**
0.1°C over range
±0.4°C to ±0.1°C using Comparison Techniques
±0.05°C
9 minutes from 0°C to 100°C
Typically 5 minutes
2 x 13mm diameter by 120mm deep
12V DC or 100V - 240V 50/60Hz
5A Anti-surge (T) 5 x 20mm
65 x 152 x 175mm
1.5 kg (3.3lbs)
Traceable Certification included UKAS Certification available

Specification Model
Temperature Range*
Set Point Resolution
Accuracy
Stability
Time to Set Point
Additional Time for best stability
Well dimensions
Power
Fuse Rating
Size
Weight
Certification

Quick Cal High Temperature
+30°C to +350°C
0.1°C over range
±0.4°C to ±0.1°C using Comparison Techniques
±0.05°C
9 minutes from Ambient to 350°C
Typically 5 minutes
1 x 25 mm diameter by 120mm deep
100-130V or 200-250V AC 50/60Hz
1.6A Quick Acting (F) 5 x 20mm
65 x 152 x 175mm
1.5 kg (3.3lbs)
Traceable Certification included UKAS Certification available

* In an ambient of 20°C.

The Quick Cal Low's minimum operating temperature is ambient dependant.

** Upper Temperature range is decreased when powered by a 12V D.C. Battery.



The apparatus Quick-Cal High and Quick-Cal Low's optional power supply are provided with an approved power cord. If the plug is not suitable for your location then the plug should be removed and replaced with an appropriate plug.

Take care to ensure the old plug is disposed safely. The cable is colour coded as follows:

COLOUR	FUNCTION
Green / Yellow	Earth (Ground)
Brown	Live (Line)
Blue	Neutral

Please ensure that your unit is correctly connected to the electricity supply.

THE APPARATUS MUST BE CORRECTLY EARTHED (GROUNDED).

The units on/off switch is located on the rear panel. Take care NOT to switch the unit off when it is hot - allow to cool first.

Accessories

Item	High	Low
Carry Case	931-22-66	931-22-66
Power Supply	n/a	935-42-20
Battery	n/a	935-42-14B
Charger		935-42-19
Inserts		
Blank Inserts	550-06-01B	560-06-01B

The company is always willing to give technical advice and assistance where appropriate. Equally, because of the programme of continual development and improvement we reserve the right to amend or alter characteristics and design without prior notice. This publication is for information only.



CE

EMC INFORMATION

This product meets the requirements of the European Directive on Electromagnetic Compatibility (EMC) 89/336/EEC as amended by EC Directive 92/31/EEC and the European Low Voltage Directive 73/25/EEC, amended by 93/68/EEC.

The product meets the susceptibility requirements of EN 50082-1, criterion B.



System Identification

Publication

Description



ISO3864

Caution
(Refer to
this leaflet)




IEC 417

Caution
Hot
Surface

The Quick Cal may be operated in any orientation or as a handheld device. For convenience a stand is provided to allow for vertical operation.



The photo on the right shows the correct position of the Quick-Cal stand.

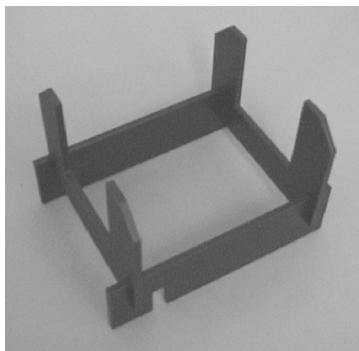

The photo on the right shows the correct assembly of the Quick-Cal stand.

Please note : The above stand is for the high temperature Quick-Cal only. The stand for the low temperature Quick-Cal includes an additional upright as the unit does not require a power entry cable.

Electrical Safety

This equipment must be correctly earthed.

This equipment is a Class 1 Appliance. A protective earth is used to ensure the conductive parts can not become live in the event of a failure of the insulation.

The protective conductor of the flexible mains cable which is coloured green / yellow MUST be connected to a suitable earth.

The Blue conductor should be connected to Neutral and the Brown conductor to Live (Line).

Warning: Internal Mains Voltage Hazard.

Do not remove the panels.

There are no user serviceable parts inside. Contact your nearest Isotech agent for repair.

Voltage transients on the supply must not exceed 2.5kV.

Conductive pollution, eg Carbon dust, must be excluded from the apparatus. EN61010 pollution degree 2.

Environmental Ratings

Operating Temperature 5 - 35°C

Relative Humidity 5 - 95%, non condensing

GUARANTEE

This instrument has been manufactured to exacting standards and is guaranteed for twelve months against electrical break-down or mechanical failure caused through defective material or workmanship, provided the failure is not the result of misuse. In the event of failure covered by this guarantee, the instrument must be returned, carriage paid, to the supplier for examination and will be replaced or repaired at our option.

FRAGILE CERAMIC AND/OR GLASS PARTS ARE NOT COVERED BY THIS GUARANTEE.

INTERFERENCE WITH, OR FAILURE TO PROPERLY MAINTAIN THIS INSTRUMENT MAY INVALIDATE THIS GUARANTEE.

RECOMMENDATION

The life of your **ISOTECH** Instrument will be prolonged if it is kept clean and free from general dust and debris.

ISOTHERMAL TECHNOLOGY LIMITED

Pine Grove, Southport, Merseyside, PR9 9AG, England
Telephone +44 (0) 1704 543830 Fax +44 (0) 1704 544799
Email info@isotech.co.uk <http://www.isotech.co.uk>